


VA\_SMArh\_C

Sample Name **VA\_SMArh\_C**  
Date collected **2018-03-08**

Pulse sequence **PROTON**  
Solvent **acetone**

Temperature **25**  
Spectrometer **chpc-nmr500a-vnmrs500**

Study owner **gmn26**  
Operator **gmn26**

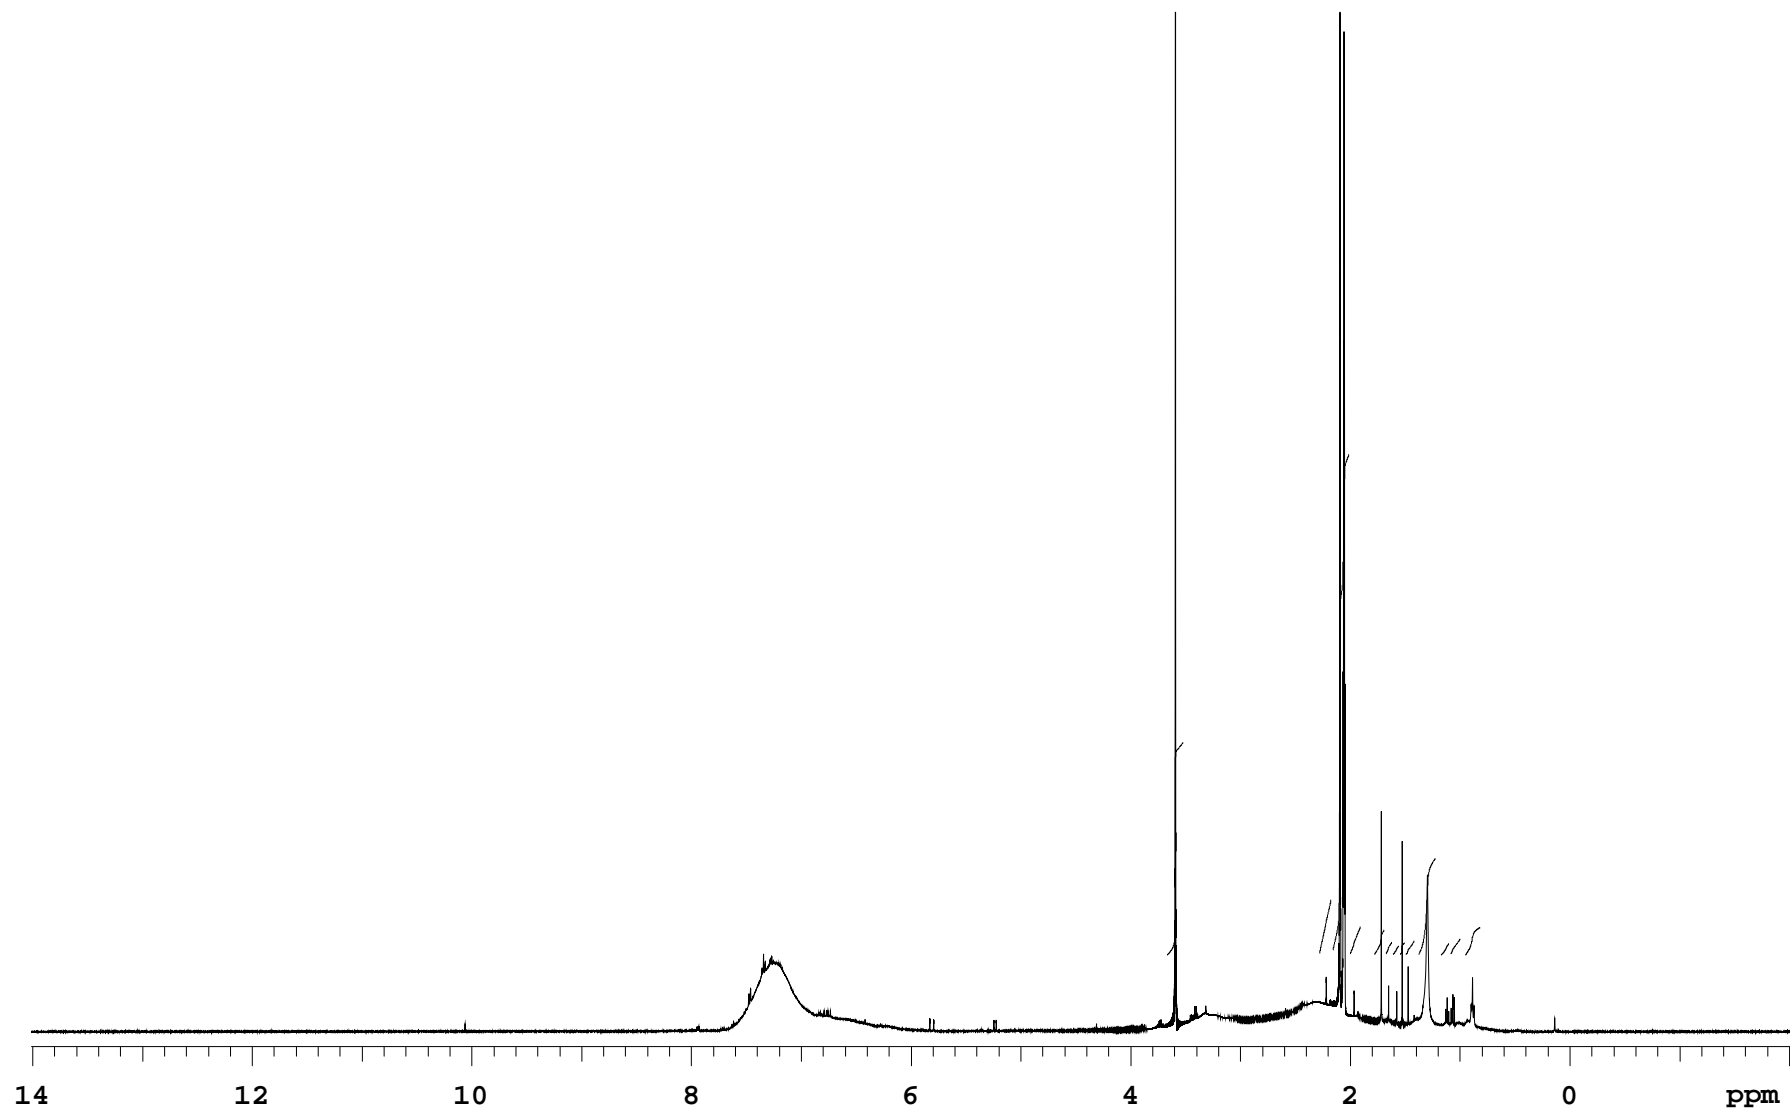

## VA\_SMArh\_C

Sample Name	VA_SMArh_C	Pulse sequence	PROTON	Temperature	25	Study owner	gmn26
Date collected	2018-03-08	Solvent	acetone	Spectrometer	chpc-nmr500a-vnmrs500	Operator	gmn26



## INTEGRAL VALUES

Integral	start(ppm)	end	value
1	3.67212	3.51612	20.573
2	2.28232	2.16691	5.649
3	2.16691	2.00407	48.393
4	2.00407	1.90333	2.789
5	1.78401	1.68327	2.563
6	1.68327	1.61481	1.350
7	1.61432	1.55466	0.918
8	1.55466	1.49989	1.258
9	1.49989	1.41089	1.509
10	1.37861	1.2187	9.391
11	1.17713	1.09449	1.233
12	1.094	0.990817	1.657
13	0.951695	0.810857	2.717

<b>SAMPLE</b>	wet	n	
date	Mar 8 2018	<b>SPECIAL</b>	
solvent	acetone		
file	/home/bath/vnmrsys	temp	25.0
/data/gmn26/VA_SMArh_C_2		gain	34
0180308_01/PROTON_01.fid		spin	0
		hst	0.008
		pw90	7.900
		alfa	10.000
<b>ACQUISITION</b>			
sw	8012.8	<b>FLAGS</b>	
at	2.045	il	n
np	32768	in	n
fb	4000	dp	y
bs	32	hs	nn
d1	1.000		
nt	8	<b>PROCESSING</b>	
ct	8		
<b>TRANSMITTER</b>		fn	65536
tn	H1	<b>DISPLAY</b>	
sfrq	500.063	sp	-1005.8
tof	500.1	wp	8012.6
tpwr	60	rfl	1006.0
pw	3.950	rfp	0
<b>DECOUPLER</b>		rp	-32.4
dn		lp	0
dof	0	<b>PLOT</b>	
dm	nnn	wc	234
decwave	W40_OneNMR	sc	8
dpwr	39	vs	183
dmf	32258	th	5
<b>PRESATURATION</b>		ai cdc ph	
satmode	n		

Plotname: PROTON\_01\_plot01

Data file /home/bath/vnmrsys/data/gmn26/VA\_SMArh\_C\_20180308\_01/PROTON\_01.fid

Plot date 2018-03-08