



54.19
53.95
53.91
53.84
53.77
53.25
-166.85
-167.97
-168.37
-168.44
-168.59
-168.72
-168.85
-168.90
-169.04
-169.80
-170.15
-170.55
-170.94
-171.27
-171.47
-171.99
-172.10
-172.43
-172.66
-172.78
-173.22
-173.34
-173.86
-174.29
-174.54
-174.71
-174.90
-175.47
-176.38
-178.28
-180.57
-183.57
-184.95
-185.40
-185.66
-186.09
-186.46
-186.59
-186.63
-186.78
-186.95
-187.10
-187.34
-187.40
-187.76
-189.03
-189.27
-189.55
-189.78
-190.32
-190.97
-191.27
-191.70
-192.03
-192.36
-192.53
-192.64
-193.80
-194.47
-194.88

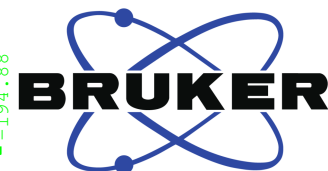

Current Data Parameters
NAME 400_TK_657_F
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20260609
Time 16.01 h
INSTRUM Avance
PROBHD Z163739_0222 (
PULPROG zg
TD 131072
SOLVENT CDCl3
NS 16
DS 4
SWH 166666.672 Hz
FIDRES 2.543132 Hz
AQ 0.3932160 sec
RG 101
DW 3.000 usec
DE 6.50 usec
TE 298.7 K
D1 1.00000000 sec
TD0 1
SFO1 376.4795375 MHz
NUC1 19F
P1 12.00 usec
PLW1 29.43499947 W

F2 - Processing parameters
SI 65536
SF 376.5077756 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00



100

50

0

-50

-100

-150

-200

-250

ppm

8.92

2.14

4.43

4.52