

19F_wide_new CDC13 {C:\Bruker\TopSpin3.2.7} LCM 12

43.23
25.84
25.61
25.60
25.13
24.47

-109.61
-109.77
-109.72

-157.88




Current Data Parameters
NAME 500_AH-TK-901-P
EXPNO 12
PROCNO 1

F2 - Acquisition Parameters
Date_ 20260604
Time 21.53
INSTRUM spect
PROBHD 5 mm CPPBBO BB
PULPROG zgflqn
TD 130840
SOLVENT CDC13
NS 16
DS 4
SWH 187500.000 Hz
FIDRES 1.433048 Hz
AQ 0.3489067 sec
RG 15.37
DW 2.667 usec
DE 18.00 usec
TE 295.2 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 470.5829518 MHz
NUC1 19F
P1 15.00 usec
PLW1 10.00000000 W

F2 - Processing parameters
SI 65536
SF 470.6300148 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

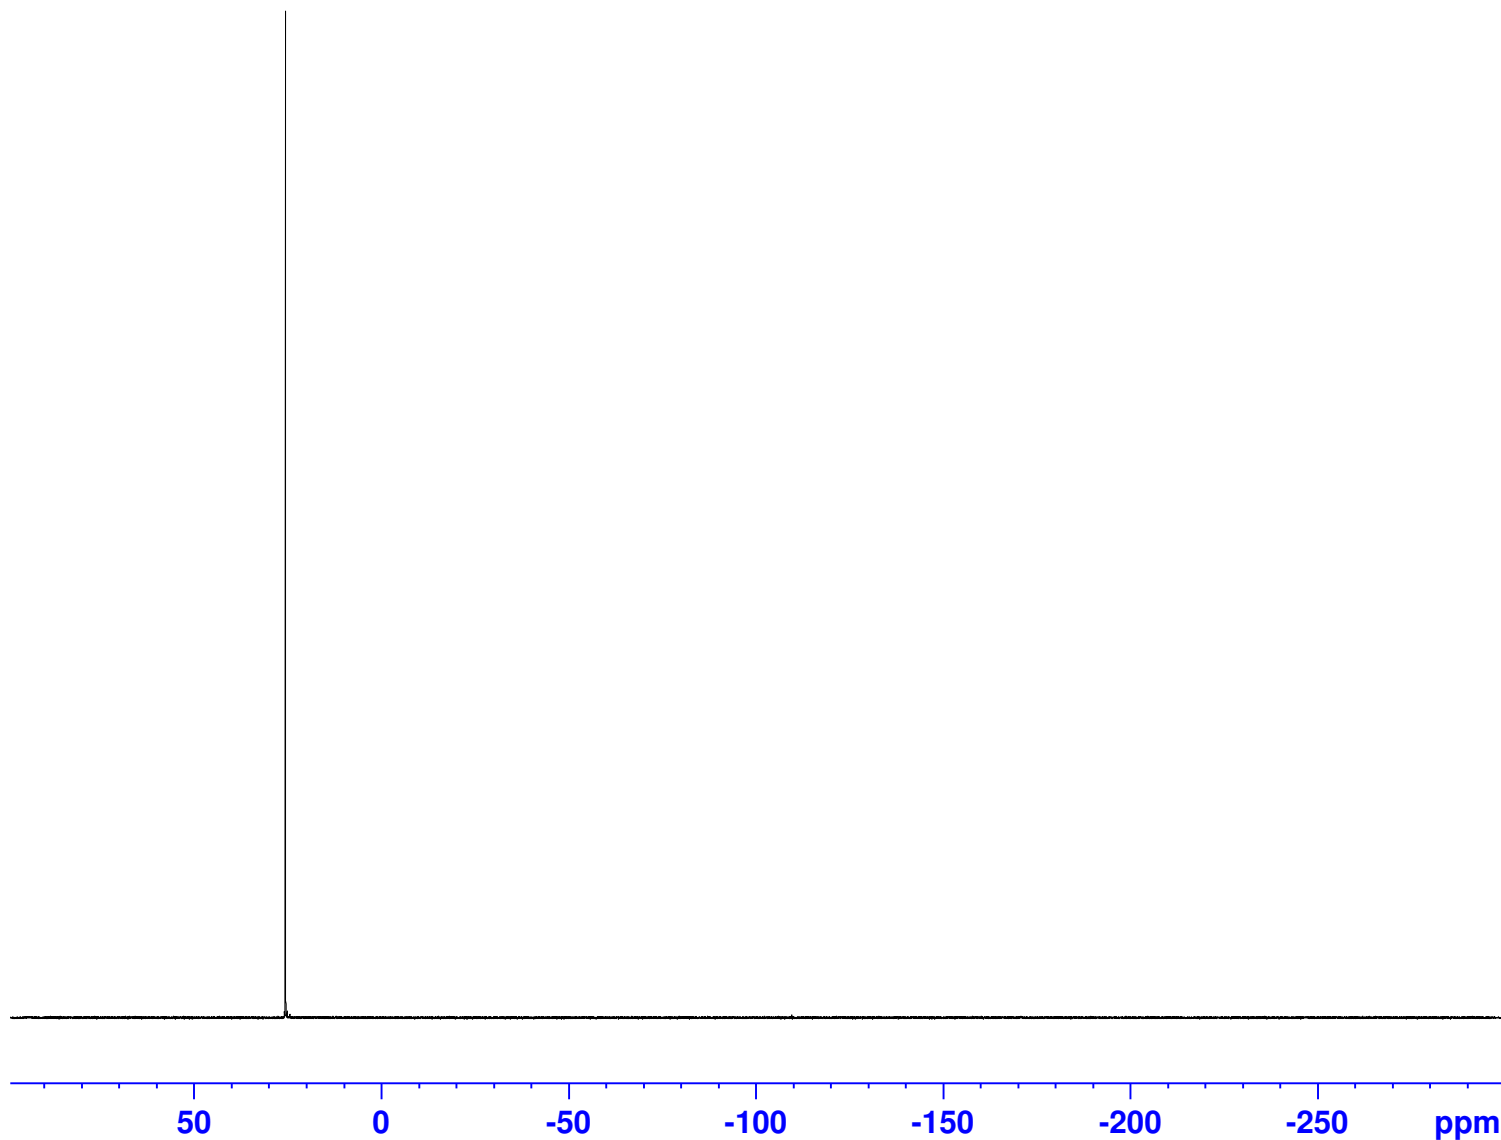

1.00