


37.07
36.81
36.70
36.62
36.09
161.14
161.36
161.67
161.83
162.04
162.50
162.92
162.94
163.04
163.23
163.43
164.06
164.30
164.53
164.83
165.01
165.22
165.43
165.82
165.89
166.09
166.38
166.50
166.68
166.81
167.15
167.26
167.41
167.78
168.06
168.15
168.56
168.92
169.13
169.58
169.88
170.34
170.53
171.23
171.38
171.46
171.57
172.33
172.87
173.01
173.43
173.48
173.75
174.15
174.48
174.70
174.87
175.13
175.21
175.56
175.69
176.39
176.68
179.08
183.13
187.23

Current Data Parameters
NAME 400_TK_653_F
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20260609
Time 15.53 h
INSTRUM Avance
PROBHD Z163739_0222 (
PULPROG zg
TD 131072
SOLVENT CDCl3
NS 16
DS 4
SWH 166666.672 Hz
FIDRES 2.543132 Hz
AQ 0.3932160 sec
RG 101
DW 3.000 usec
DE 6.50 usec
TE 298.7 K
D1 1.00000000 sec
TD0 1
SFO1 376.4795375 MHz
NUC1 19F
P1 12.00 usec
PLW1 29.43499947 W

F2 - Processing parameters
SI 65536
SF 376.5077756 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

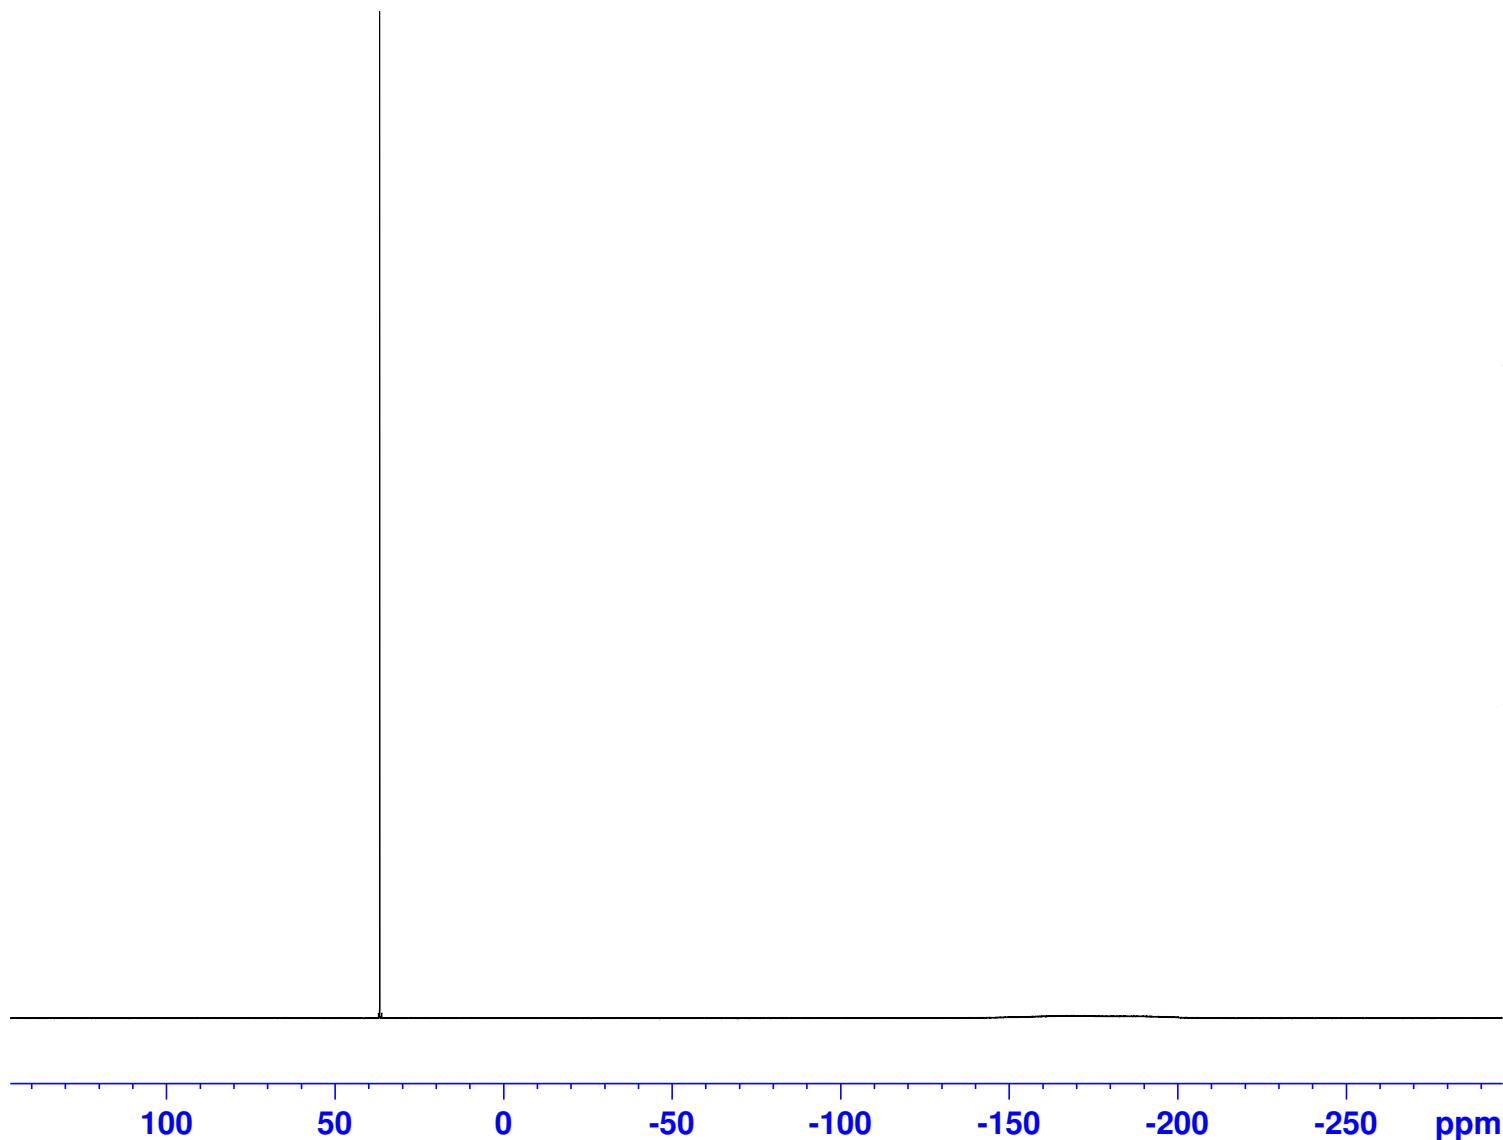

6.57

3.30

7.94

2.19