


-16.80
-44.97
-79.19
-90.31
-92.15
-93.30
-93.99
-94.68
-94.76
-95.70
-95.87
-95.99
-96.06
-96.23
-96.31
-96.41
-96.46
-96.48
-96.51
-96.53
-96.56
-96.62
-96.70
-96.76
-96.96
-97.75
-97.84
-97.92
-98.18
-99.23
-100.67
-104.71
-107.85
-108.21
-112.97
-113.14
-117.97
-118.88
-118.92
-121.13
-123.46
-123.90
-124.11
-124.29
-125.56
-126.23
-126.65
-127.45
-134.70
-134.99
-135.71
-193.70
-195.65
-196.38
-196.90
-197.20
-197.31
-197.49
-197.70
-198.33
-199.11
-199.26
-199.35
-199.74
-201.24
-201.32

Current Data Parameters
NAME 400_TK_659_F
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20260611
Time 16.58 h
INSTRUM Avance
PROBHD Z163739_0222 (
PULPROG zgig
TD 131072
SOLVENT CDCl3
NS 16
DS 4
SWH 90909.094 Hz
FIDRES 1.387163 Hz
AQ 0.7208960 sec
RG 101
DW 5.500 usec
DE 6.50 usec
TE 298.5 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 376.4701248 MHz
NUC1 19F
P1 12.00 usec
PLW1 29.43499947 W
SFO2 400.1416006 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 21.11599922 W
PLW12 0.16684000 W

F2 - Processing parameters
SI 65536
SF 376.5077756 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

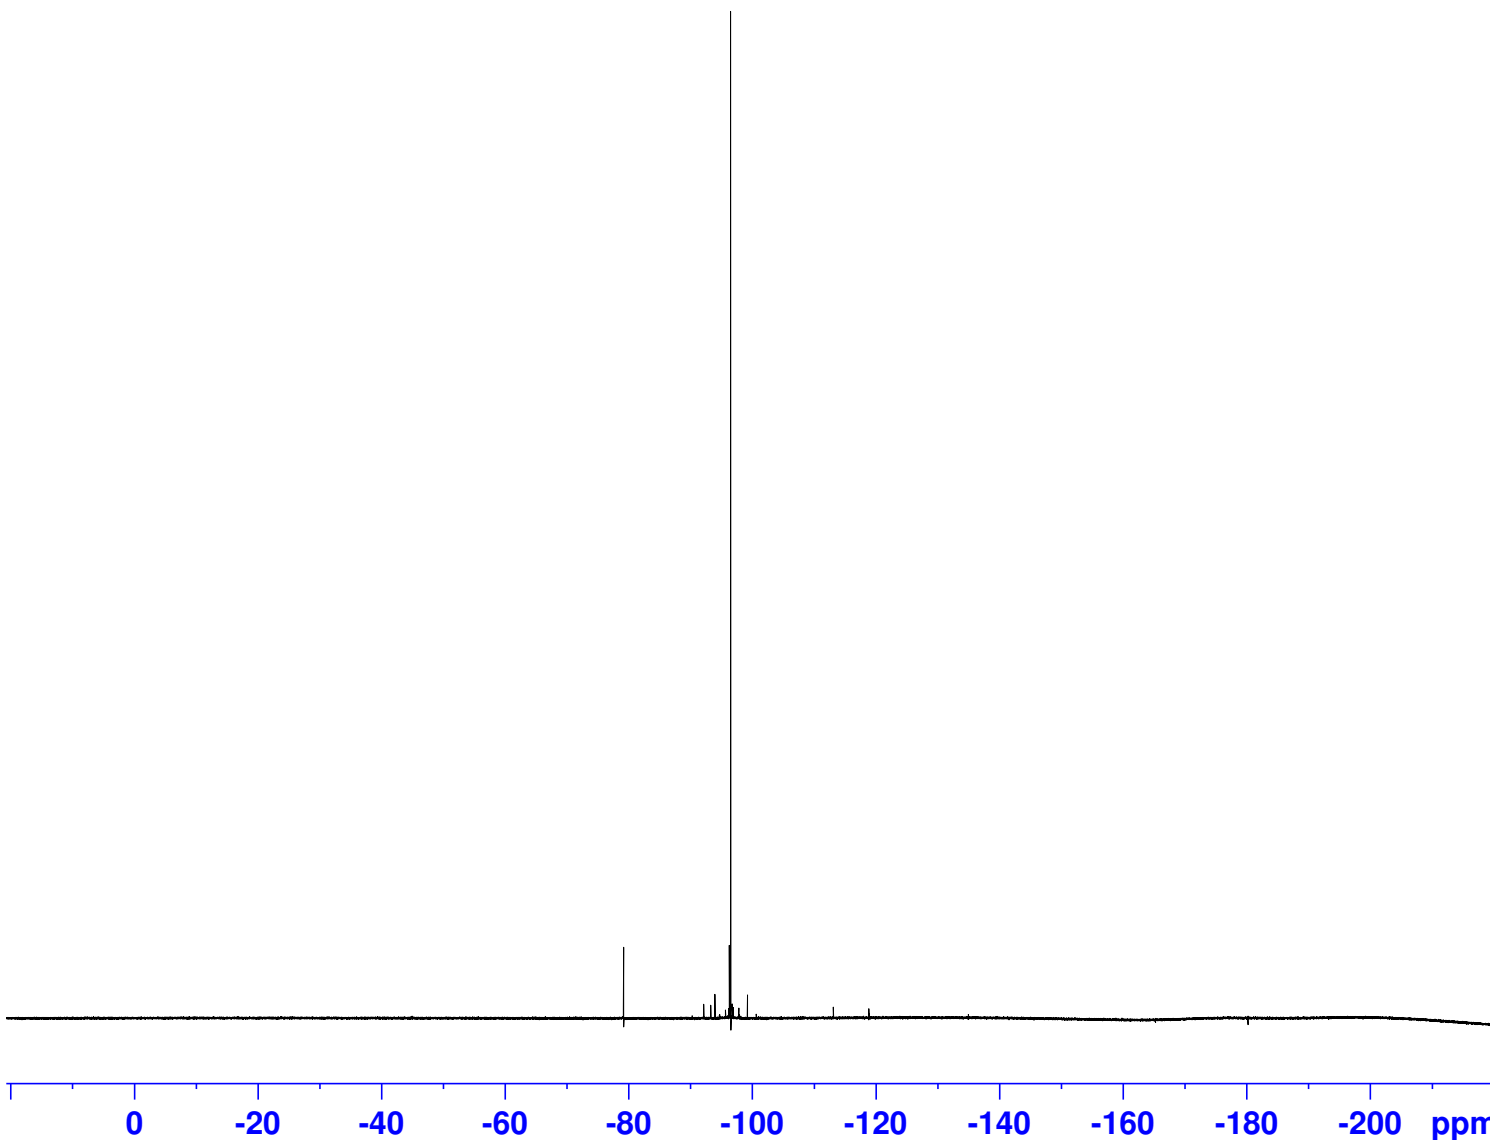

1.25

8.61

0.61

0.24

9.30