



-98.74
 -98.79
 -98.89
 -157.85
 -159.67
 -161.86
 -162.08
 -162.26
 -162.35
 -162.47
 -162.47
 -162.83
 -162.98
 -163.02
 -163.34
 -163.48
 -163.70
 -163.75
 -164.24
 -164.41
 -164.45
 -164.65
 -164.93
 -164.98
 -165.25
 -165.46
 -165.57
 -165.62
 -165.70
 -165.81
 -165.84
 -165.87
 -165.91
 -165.99
 -166.08
 -166.20
 -166.32
 -166.83
 -167.04
 -167.13
 -167.21
 -167.32
 -167.46
 -167.80
 -167.93
 -168.55
 -168.64
 -168.83
 -169.84
 -170.11
 -179.35
 -179.40
 -214.98
 -215.89
 -216.02
 -216.27
 -216.81
 -217.07
 -217.32
 -217.94
 -218.23
 -218.57
 -218.66
 -218.79
 -219.10
 -219.37

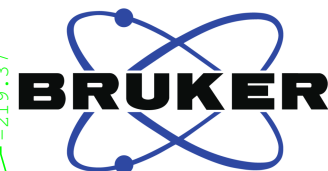

Current Data Parameters
 NAME 400_TK_622_F
 EXPNO 12
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20260519
 Time 23.14 h
 INSTRUM Avance
 PROBHD Z163739_0222 (
 PULPROG zgig
 TD 131072
 SOLVENT CDCl3
 NS 16
 DS 4
 SWH 90909.094 Hz
 FIDRES 1.387163 Hz
 AQ 0.7208960 sec
 RG 101
 DW 5.500 usec
 DE 6.50 usec
 TE 298.8 K
 D1 1.00000000 sec
 D11 0.03000000 sec
 TD0 1
 SFO1 376.4701248 MHz
 NUC1 19F
 P1 12.00 usec
 PLW1 29.43499947 W
 SFO2 400.1416006 MHz
 NUC2 1H
 CPDPRG[2] waltz16
 PCPD2 90.00 usec
 PLW2 21.11599922 W
 PLW12 0.16684000 W

F2 - Processing parameters
 SI 65536
 SF 376.5077756 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00

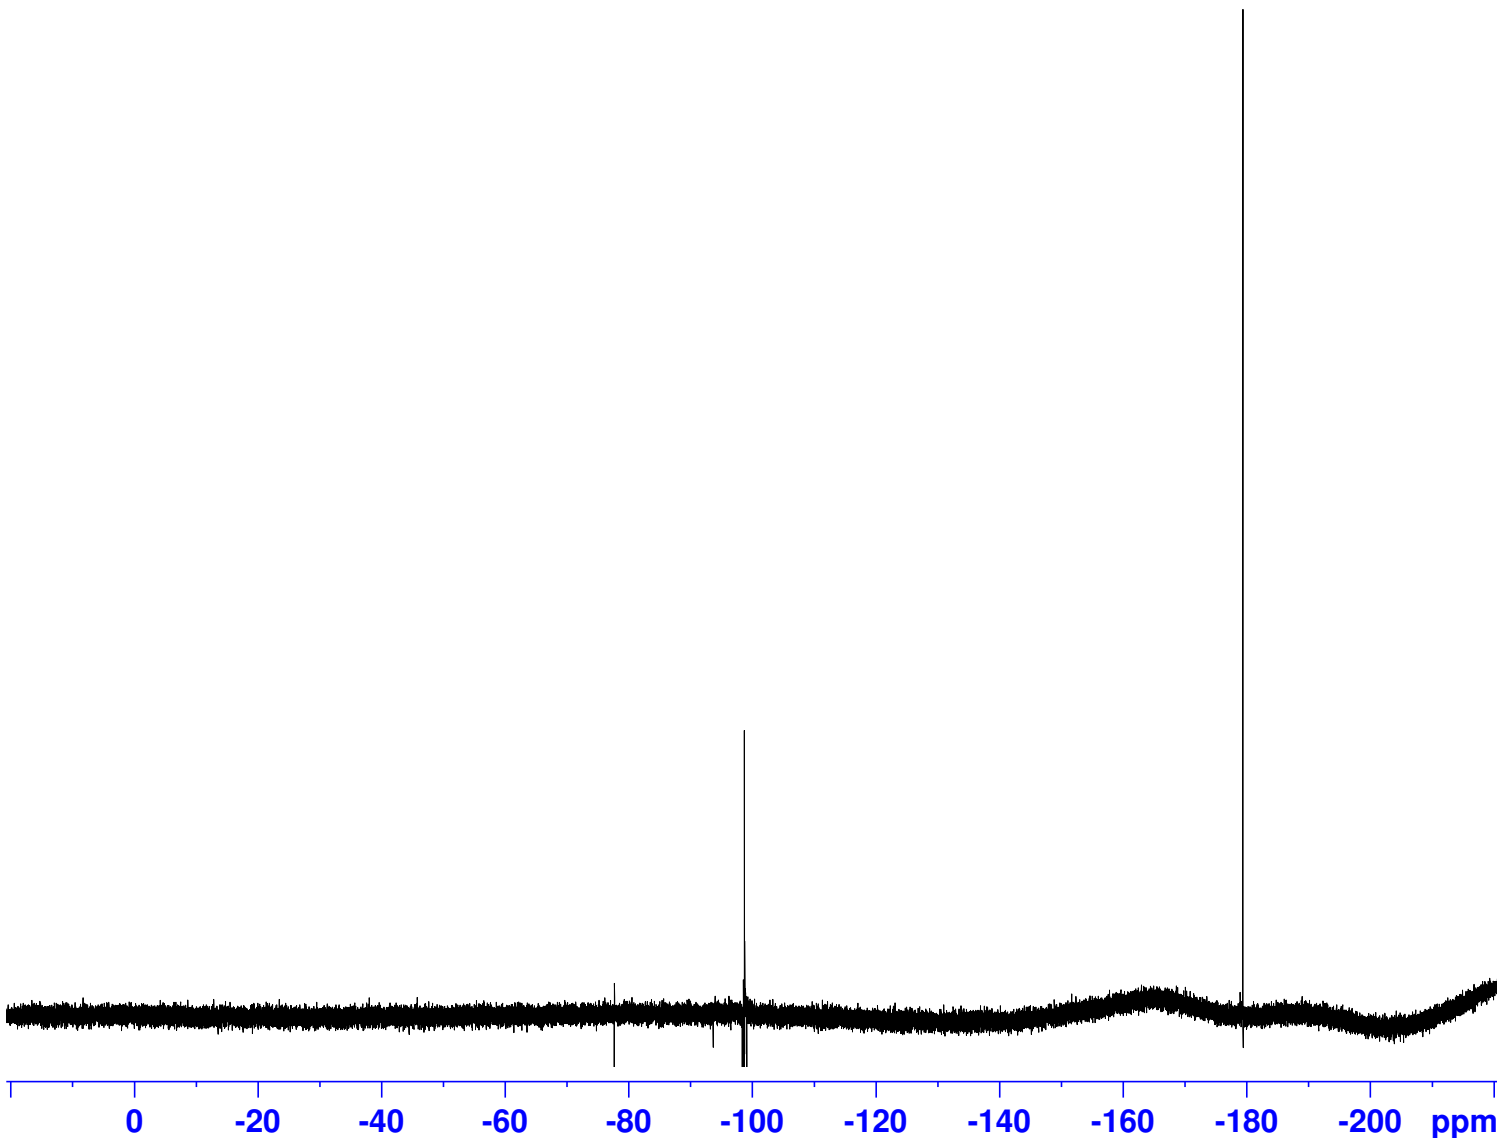

.06

.98

.95

.14