

— 2.26  
— 4.74


-97.83  
-97.88  
-98.04  
-98.11  
-98.15  
-98.56  
-110.48  
-118.15  
-118.68  
-122.09  
-123.15  
-123.56  
-125.61  
-126.36  
-126.89  
-127.89  
-128.59  
-129.33  
-129.77  
-129.98  
-130.70  
-132.15  
-133.26  
-134.43  
-139.28  
-181.60  
-182.42  
-184.56  
-188.69  
-190.11  
-191.83  
-192.63  
-195.05  
-195.57  
-196.57  
-196.77  
-196.88  
-198.04  
-198.13  
-198.91



Current Data Parameters  
NAME 400\_TK\_534\_F  
EXPNO 11  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20260203  
Time 17.27 h  
INSTRUM Avance  
PROBHD Z163739\_0222 (  
PULPROG zgig  
TD 131072  
SOLVENT CDCl3  
NS 16  
DS 4  
SWH 90909.094 Hz  
FIDRES 1.387163 Hz  
AQ 0.7208960 sec  
RG 101  
DW 5.500 usec  
DE 6.50 usec  
TE 300.4 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 376.4701248 MHz  
NUC1 19F  
P1 12.00 usec  
PLW1 29.43499947 W  
SFO2 400.1416006 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 21.11599922 W  
PLW12 0.16684000 W

F2 - Processing parameters  
SI 65536  
SF 376.5077756 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

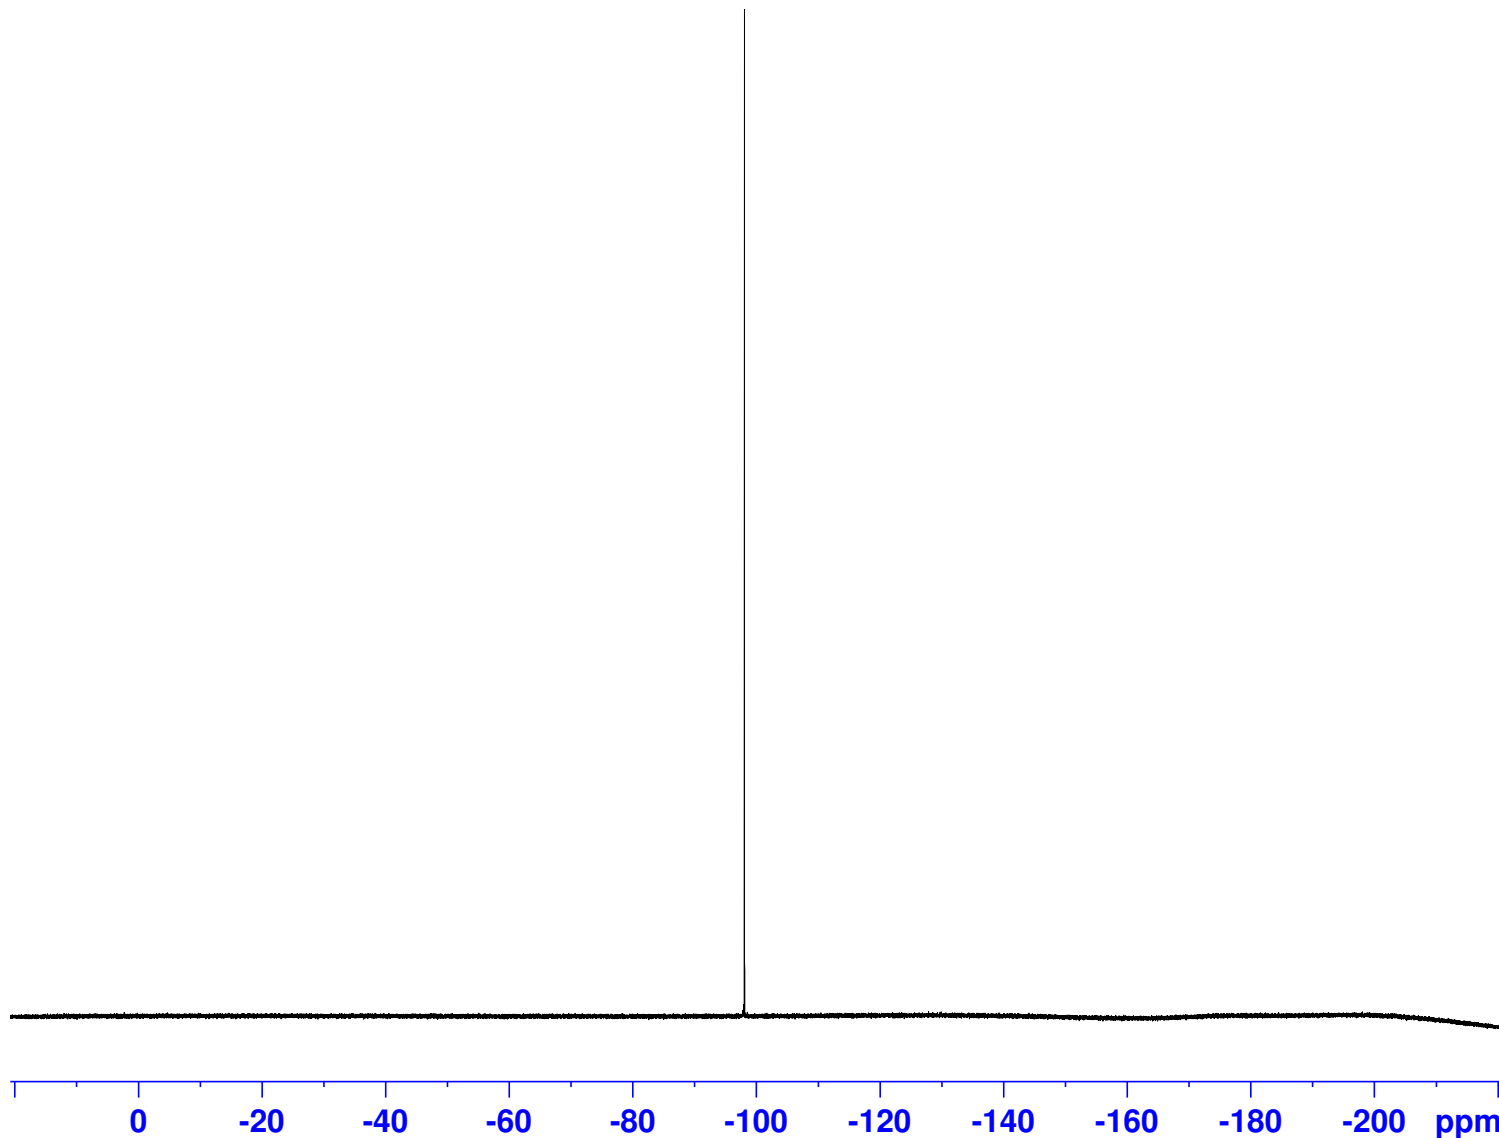

0.89

7.32

1.79