

-81.46
-96.01
-98.11
-98.12
-98.14
-98.17
-98.21
-98.29
-98.30
-98.31
-98.39
-98.41
-98.42
-98.46
-98.62
-98.84
-98.86
-98.87
-116.28
-121.19
-121.68
-122.43
-125.43
-126.05
-131.53
-134.82
-140.87


-193.06
-195.19
-196.01
-196.14
-196.36
-197.41
-198.33
-198.76
-199.13
-199.71
-200.45
-201.20



Current Data Parameters
NAME 400_TK_641_F3
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20260629
Time 17.27 h
INSTRUM Avance
PROBHD Z163739_0222 (
PULPROG zgig
TD 131072
SOLVENT CDCl3
NS 16
DS 4
SWH 90909.094 Hz
FIDRES 1.387163 Hz
AQ 0.7208960 sec
RG 101
DW 5.500 usec
DE 6.50 usec
TE 298.4 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 376.4701248 MHz
NUC1 19F
P1 12.00 usec
PLW1 29.43499947 W
SFO2 400.1416006 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 21.11599922 W
PLW12 0.16684000 W

F2 - Processing parameters
SI 65536
SF 376.5077756 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

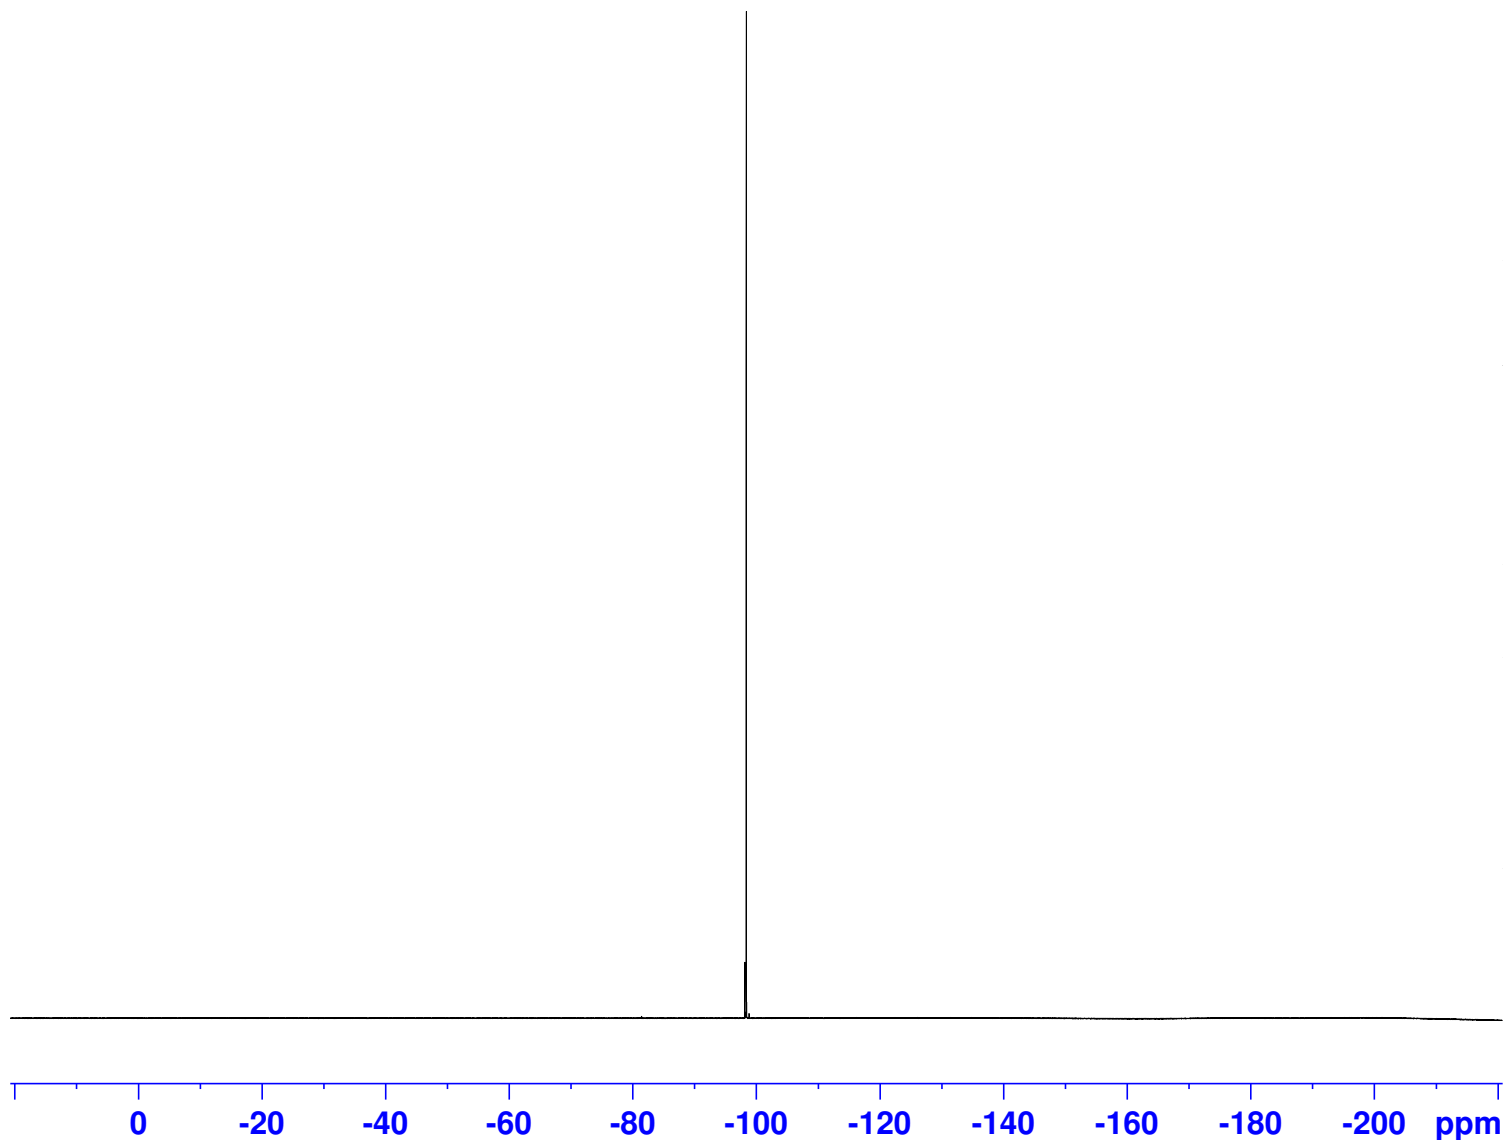

1.03

2.02

6.94