

-2.59
-3.32


-80.08
-91.22
-95.92
-97.00
-97.24
-97.26
-97.28
-97.31
-97.33
-97.34
-97.39
-97.44
-97.46
-97.74
-110.70
-113.22
-117.08
-117.10
-120.64
-122.33
-123.07
-124.29
-125.00
-125.07
-126.56
-127.05
-128.03
-129.05
-129.63
-129.97
-131.96
-132.72
-132.90
-135.79
-136.34
-177.98
-191.77
-195.85
-196.63
-196.98
-197.16
-197.47
-197.58
-198.16
-198.58
-198.75
-199.00
-199.14



Current Data Parameters
NAME 400_TK_636_F
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20260527
Time 17.47 h
INSTRUM Avance
PROBHD Z163739_0222 (
PULPROG zgig
TD 131072
SOLVENT CDCl3
NS 16
DS 4
SWH 90909.094 Hz
FIDRES 1.387163 Hz
AQ 0.7208960 sec
RG 101
DW 5.500 usec
DE 6.50 usec
TE 298.3 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 376.4701248 MHz
NUC1 19F
P1 12.00 usec
PLW1 29.43499947 W
SFO2 400.1416006 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 21.11599922 W
PLW12 0.16684000 W

F2 - Processing parameters
SI 65536
SF 376.5077756 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

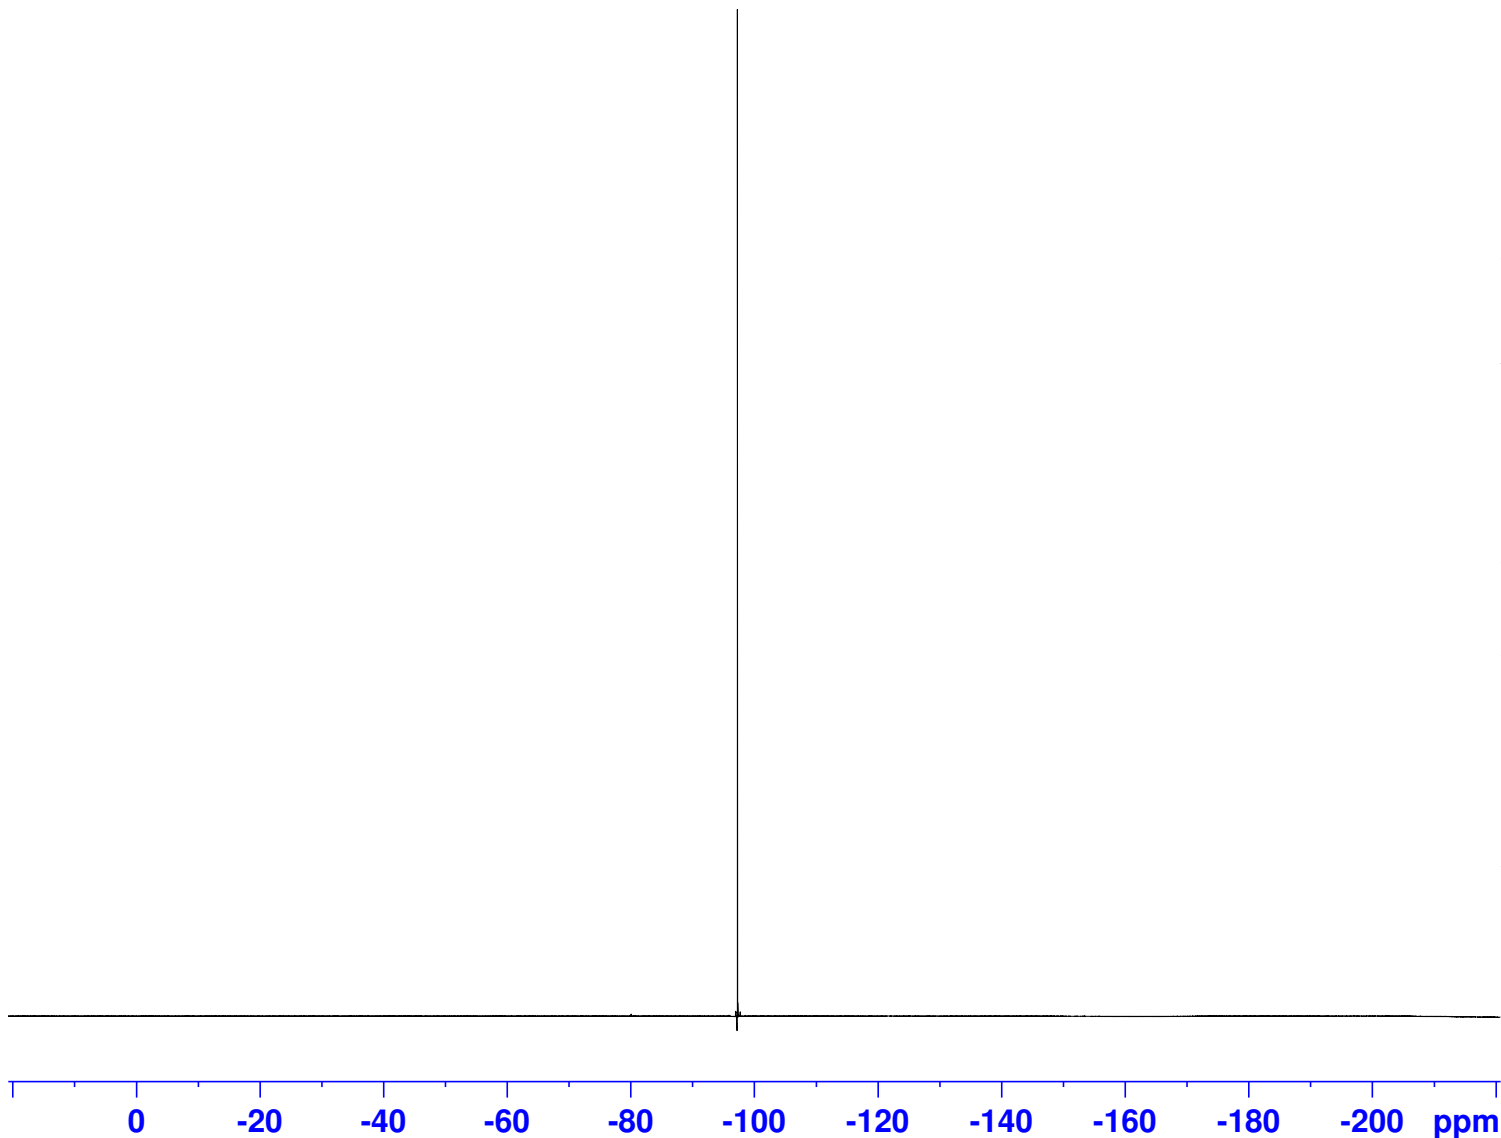

8.47

0.83

0.70