


1.10
-1.93
-9.94
-18.85
-79.29
-96.39
-96.46
-96.49
-96.57
-96.62
-96.65
-96.68
-96.69
-96.70
-96.72
-96.92
-97.13
-97.34
-108.72
-112.99
-115.48
-122.03
-122.23
-122.70
-123.01
-124.06
-124.51
-124.95
-125.13
-126.06
-126.26
-126.34
-126.59
-127.39
-127.59
-130.27
-131.55
-132.36
-132.56
-132.91
-191.75
-192.74
-194.56
-195.30
-195.53
-196.06
-196.18
-196.77
-197.05
-197.30
-197.42
-197.76
-198.23
-198.28
-198.54
-198.84
-198.99
-199.04
-199.29
-199.34
-199.75
-199.82
-200.09
-200.36
-200.75
-200.89

Current Data Parameters
NAME 400_TK_640_F3
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20260605
Time 17.19 h
INSTRUM Avance
PROBHD Z163739_0222 (
PULPROG zgig
TD 131072
SOLVENT CDCl3
NS 16
DS 4
SWH 90909.094 Hz
FIDRES 1.387163 Hz
AQ 0.7208960 sec
RG 101
DW 5.500 usec
DE 6.50 usec
TE 300.8 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 376.4701248 MHz
NUC1 19F
P1 12.00 usec
PLW1 29.43499947 W
SFO2 400.1416006 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 21.11599922 W
PLW12 0.16684000 W

F2 - Processing parameters
SI 65536
SF 376.5077756 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

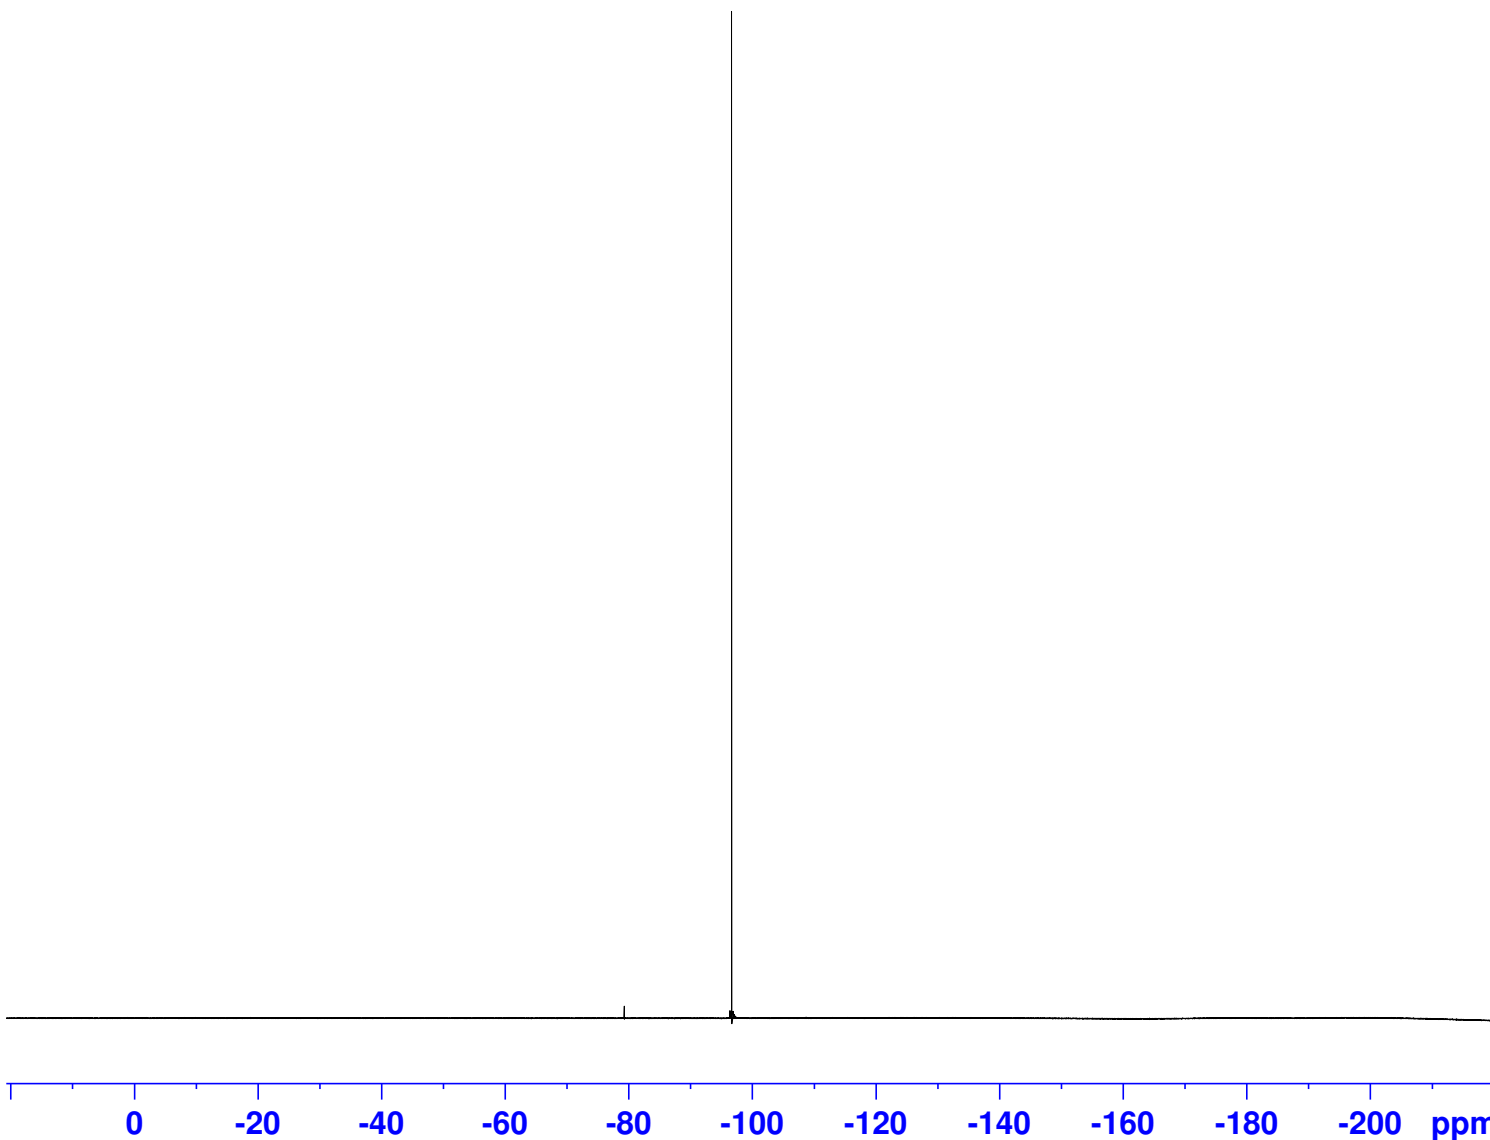

0.39

6.79

5.22

7.60