




6.26
-34.54
-80.26
-95.33
-96.84
-97.11
-97.18
-97.30
-97.40
-97.51
-97.57
-97.62
-97.65
-97.68
-97.69
-97.72
-97.73
-98.13
-105.70
-107.36
-107.61
-107.66
-107.71
-107.90
-107.94
-108.03
-108.44
-108.48
-109.04
-109.11
-109.75
-111.72
-111.94
-112.54
-113.47
-114.60
-114.90
-115.04
-115.84
-116.53
-118.63
-119.59
-119.77
-121.43
-122.14
-123.79
-123.93
-125.00
-125.28
-126.20
-126.40
-126.60
-128.37
-134.30
-178.96
-184.68
-193.60
-194.40
-194.60
-194.80
-195.84
-196.59
-197.19
-197.87
-198.65
-199.60

Current Data Parameters
NAME 400_TK_668_F
EXPNO 12
PROCNO 1

F2 - Acquisition Parameters
Date_ 20260619
Time 16.55 h
INSTRUM Avance
PROBHD Z163739_0222 (
PULPROG zgig
TD 131072
SOLVENT CDCl3
NS 16
DS 4
SWH 90909.094 Hz
FIDRES 1.387163 Hz
AQ 0.7208960 sec
RG 101
DW 5.500 usec
DE 6.50 usec
TE 302.3 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 376.4701248 MHz
NUC1 19F
P1 12.00 usec
PLW1 29.43499947 W
SFO2 400.1416006 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 21.11599922 W
PLW12 0.16684000 W

F2 - Processing parameters
SI 65536
SF 376.5077756 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

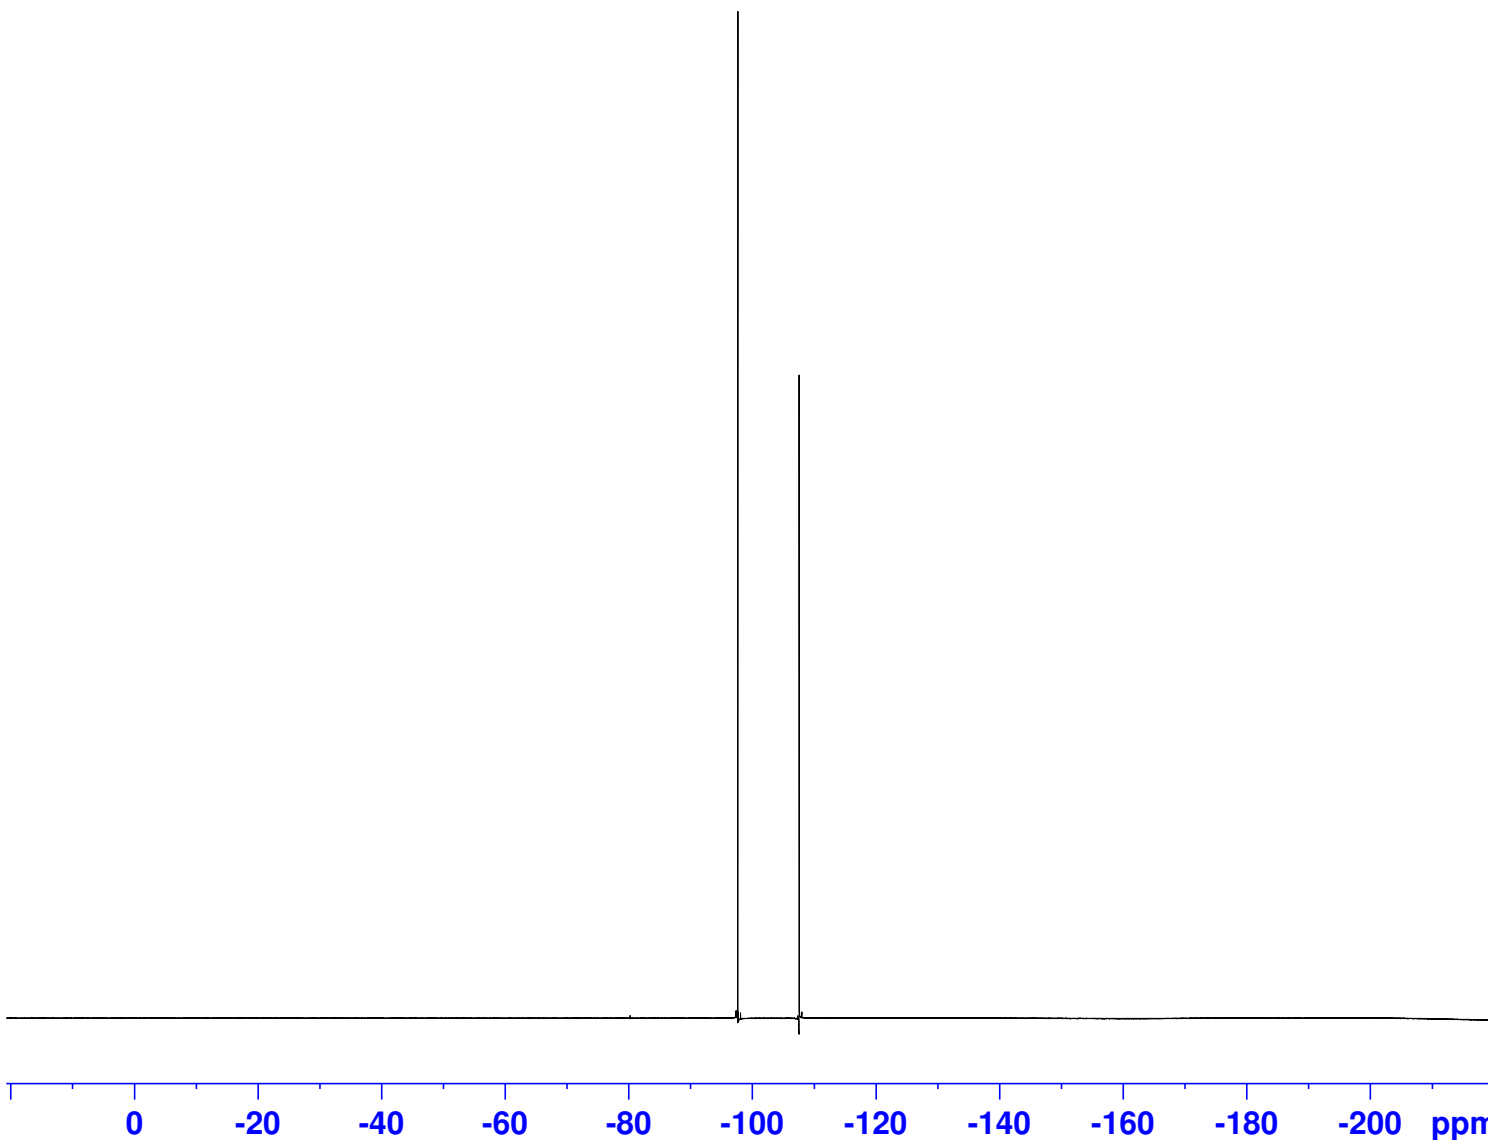

5.85

5.82

8.33