


mlo462_dms0

Sample Name **mlo462_dms0**
Date collected **2019-05-28**

Pulse sequence **PROTON**
Solvent **dms0**


Temperature **25**
Spectrometer **chpc-nmr500a-vnmrs500**

Study owner **mlo22**
Operator **mlo22**

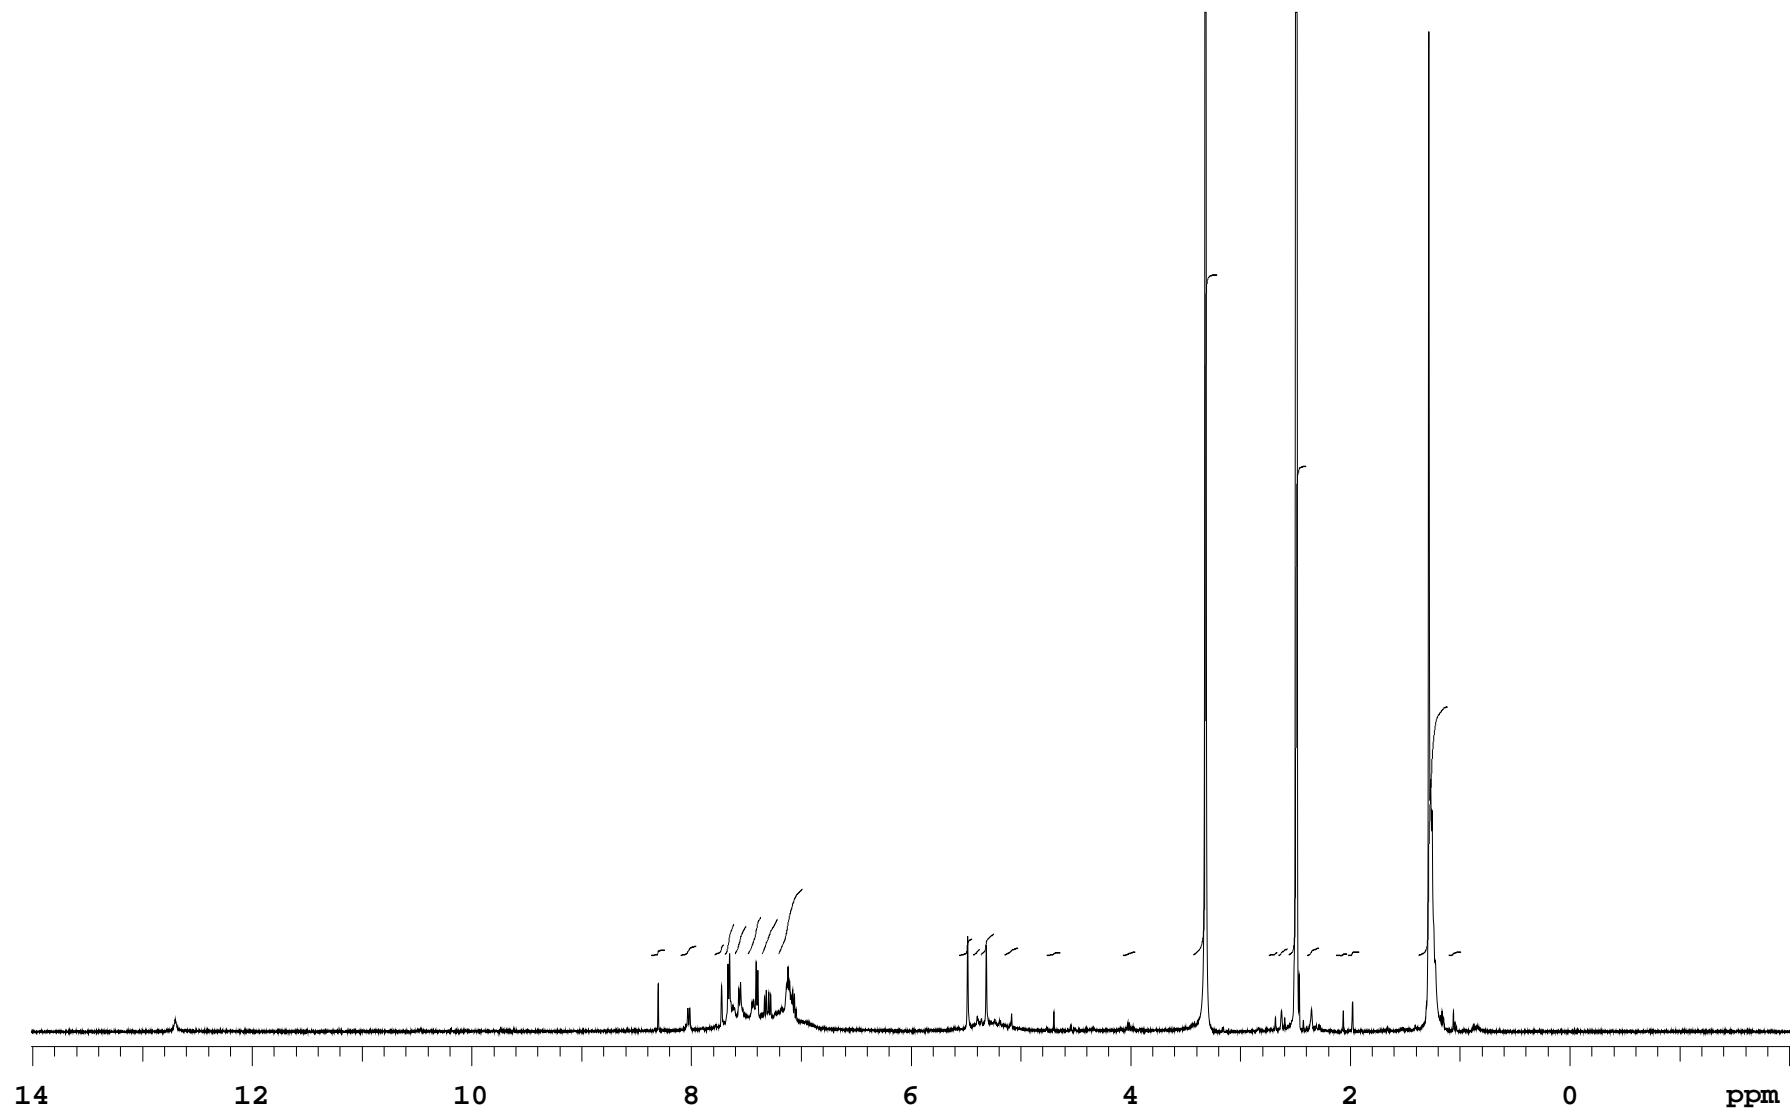

mlo462_dms0

Sample Name	mlo462_dms0	Pulse sequence	PROTON	Temperature	25	Study owner	mlo22
Date collected	2019-05-28	Solvent	dms0	Spectrometer	chpc-nmr500a-vnmrs500	Operator	mlo22

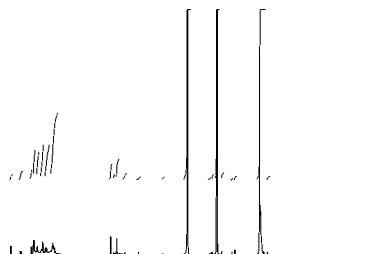

INTEGRAL VALUES

Integral	start(ppm)	end	value
1	8.37333	8.2364	0.307
2	8.10143	7.94885	0.525
3	7.79725	7.70238	0.634
4	7.70238	7.60848	1.863
5	7.60848	7.49405	1.765
6	7.49307	7.36494	2.225
7	7.36396	7.21334	2.117
8	7.21041	6.98252	3.892
9	5.5604	5.43716	0.972
10	5.43619	5.36772	0.395
11	5.36772	5.23959	1.294
12	5.15059	5.01953	0.429
13	4.76718	4.63417	0.142
14	4.0708	3.95343	0.208
15	3.43407	3.20912	39.243
16	2.74844	2.65846	0.146
17	2.65748	2.5675	0.375
18	2.56652	2.39438	28.253
19	2.39438	2.2819	0.448
20	2.13128	2.02467	0.069
21	2.02467	1.91317	0.185
22	1.38208	1.10724	14.335
23	1.10724	0.984003	0.178

SAMPLE

date May 28 2019
solvent dms0
file /home/bath/vnmrsys
/data/mlo22/mlo462_dms0_
20190528_01/PROTON_01.f
d

PRESATURATION

satmode n
wet n

SPECIAL

temp 25.0
gain 42
spin 0
hst 0.008
pw90 7.800
alfa 10.000

ACQUISITION

sw 8012.8
at 2.045
np 32768
fb 4000
bs 32
d1 1.000
nt 8
ct 8

FLAGS

il n
in n
dp y
hs nn

TRANSMITTER

tn H1
sfrq 500.062
tof 500.1
tpwr 60
pw 3.900

PROCESSING

fn not used

DISPLAY

sp -1005.5
wp 8012.3
rfi 1006.0
rfp 0
rp 136.1
lp 0

DECOUPLER

dn C13
dof 0
dm nnn
decwave W40_OneNMR
dpwr 38
dmf 32258

PLOT

wc 234
sc 8
vs 232
th 4
ai cdc ph

Plotname: PROTON_01_plot01

Data file /home/bath/vnmrsys/data/mlo22/mlo462_dms0_20190528_01/PROTON_01.fid

Plot date 2019-05-28