


krt37

Sample Name **krt37**
Date collected **2018-07-09**

Pulse sequence **PROTON**
Solvent **dms**

Temperature **25**
Spectrometer **chpc-nmr500a-vnmrs500**

Study owner **mlo22**
Operator **mlo22**

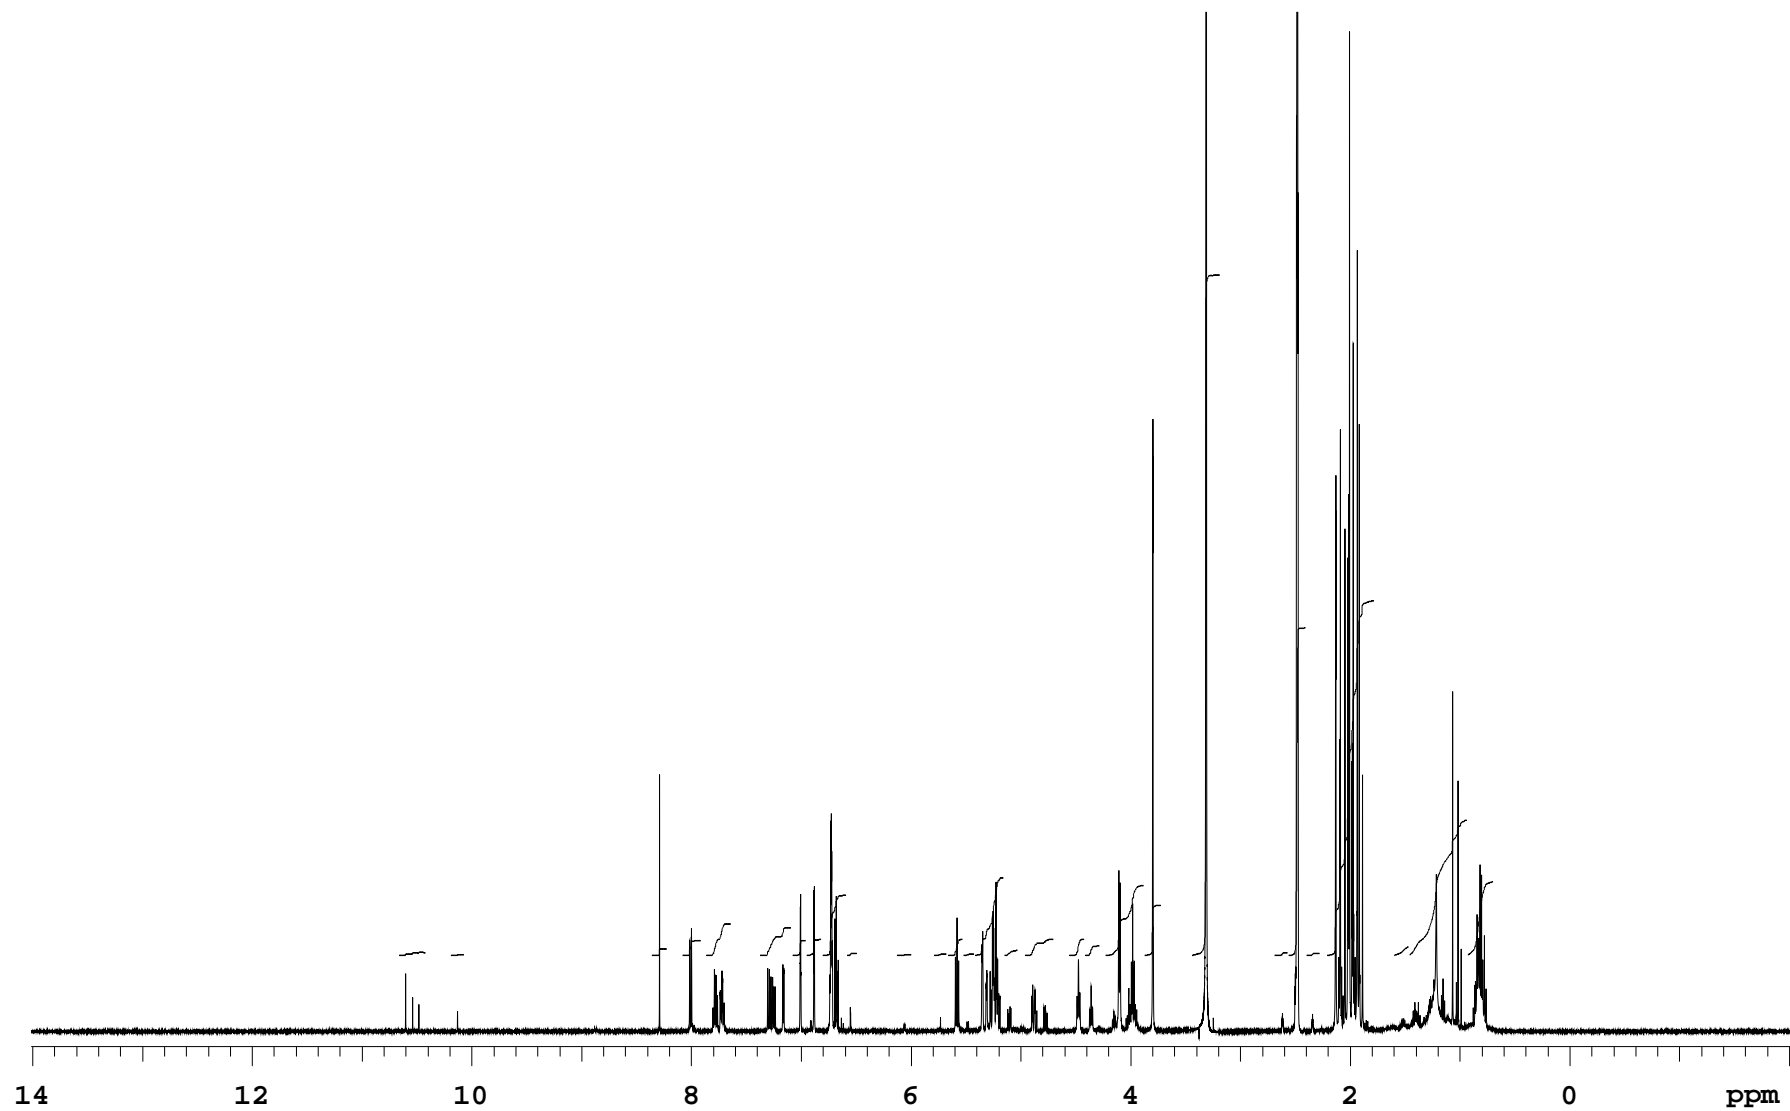


krt37

Sample Name **krt37**
Date collected **2018-07-09**

Pulse sequence **PROTON**
Solvent **dmsO**

Temperature **25**
Spectrometer **chpc-nmr500a-vnmrs500**

Study owner **mlo22**
Operator **mlo22**

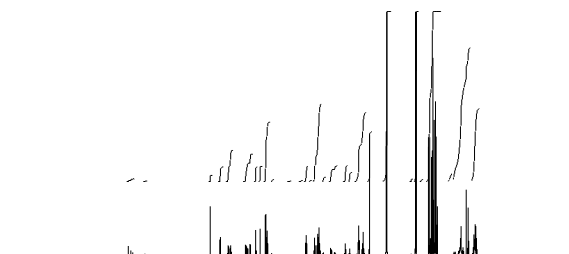

INTEGRAL VALUES

Integral	start(ppm)	end	value
1	10.6699	10.42	0.140
2	10.1961	10.0675	0.026
3	8.36127	8.22287	0.312
4	8.08741	7.91332	0.734
5	7.87225	7.63703	1.556
6	7.3754	7.09079	1.360
7	7.08199	6.95729	0.740
8	6.95729	6.81254	0.780
9	6.81205	6.58759	2.967
10	6.58759	6.48685	0.093
11	6.12742	5.99441	0.034
12	5.79586	5.67018	0.054
13	5.66578	5.52641	0.799
14	5.52641	5.42176	0.071
15	5.42127	5.15525	3.833
16	5.15476	5.0281	0.251
17	4.96844	4.69801	0.779
18	4.55864	4.4178	0.783
19	4.41731	4.28137	0.499
20	4.231	3.87792	3.445
21	3.87792	3.7185	2.477
22	3.44074	3.18302	33.562
23	2.68862	2.56588	0.147
24	2.56539	2.40108	16.161
25	2.40108	2.2754	0.107
26	2.21623	1.77856	17.515
27	1.59811	1.46705	0.433
28	1.46656	0.933528	6.705
29	0.933528	0.696842	3.639

SAMPLE	wet	n
date	Jul 9 2018	
solvent	dmsO	
file	/home/bath/vnmrsys /data/mlo22/krt37_201807 09_01/PROTON_01.fid	
ACQUISITION	temp	25.0
	gain	36
	spin	0
	hst	0.008
	pw90	7.800
	alfa	10.000
FLAGS	il	n
	in	n
	dp	y
	hs	nn
PROCESSING		
	fn	65536
DISPLAY	sp	-1005.8
	wp	8012.6
	rfl	1006.0
	rfp	0
	rp	-53.8
	lp	0
PLOT	wc	234
	sc	8
	vs	274
	th	3
	ai cdc ph	
PRESATURATION		
satmode	n	

Plotname: PROTON_01_plot01

Data file /home/bath/vnmrsys/data/mlo22/krt37_20180709_01/PROTON_01.fid

Plot date 2018-07-09