


mlo162_column

Sample Name **mlo162_column**
Date collected **2017-08-18**

Pulse sequence **PROTON**
Solvent **cdcl3**


Temperature **25**
Spectrometer **chpc-nmr500a-vnmrs500**

Study owner **mlo22**
Operator **mlo22**

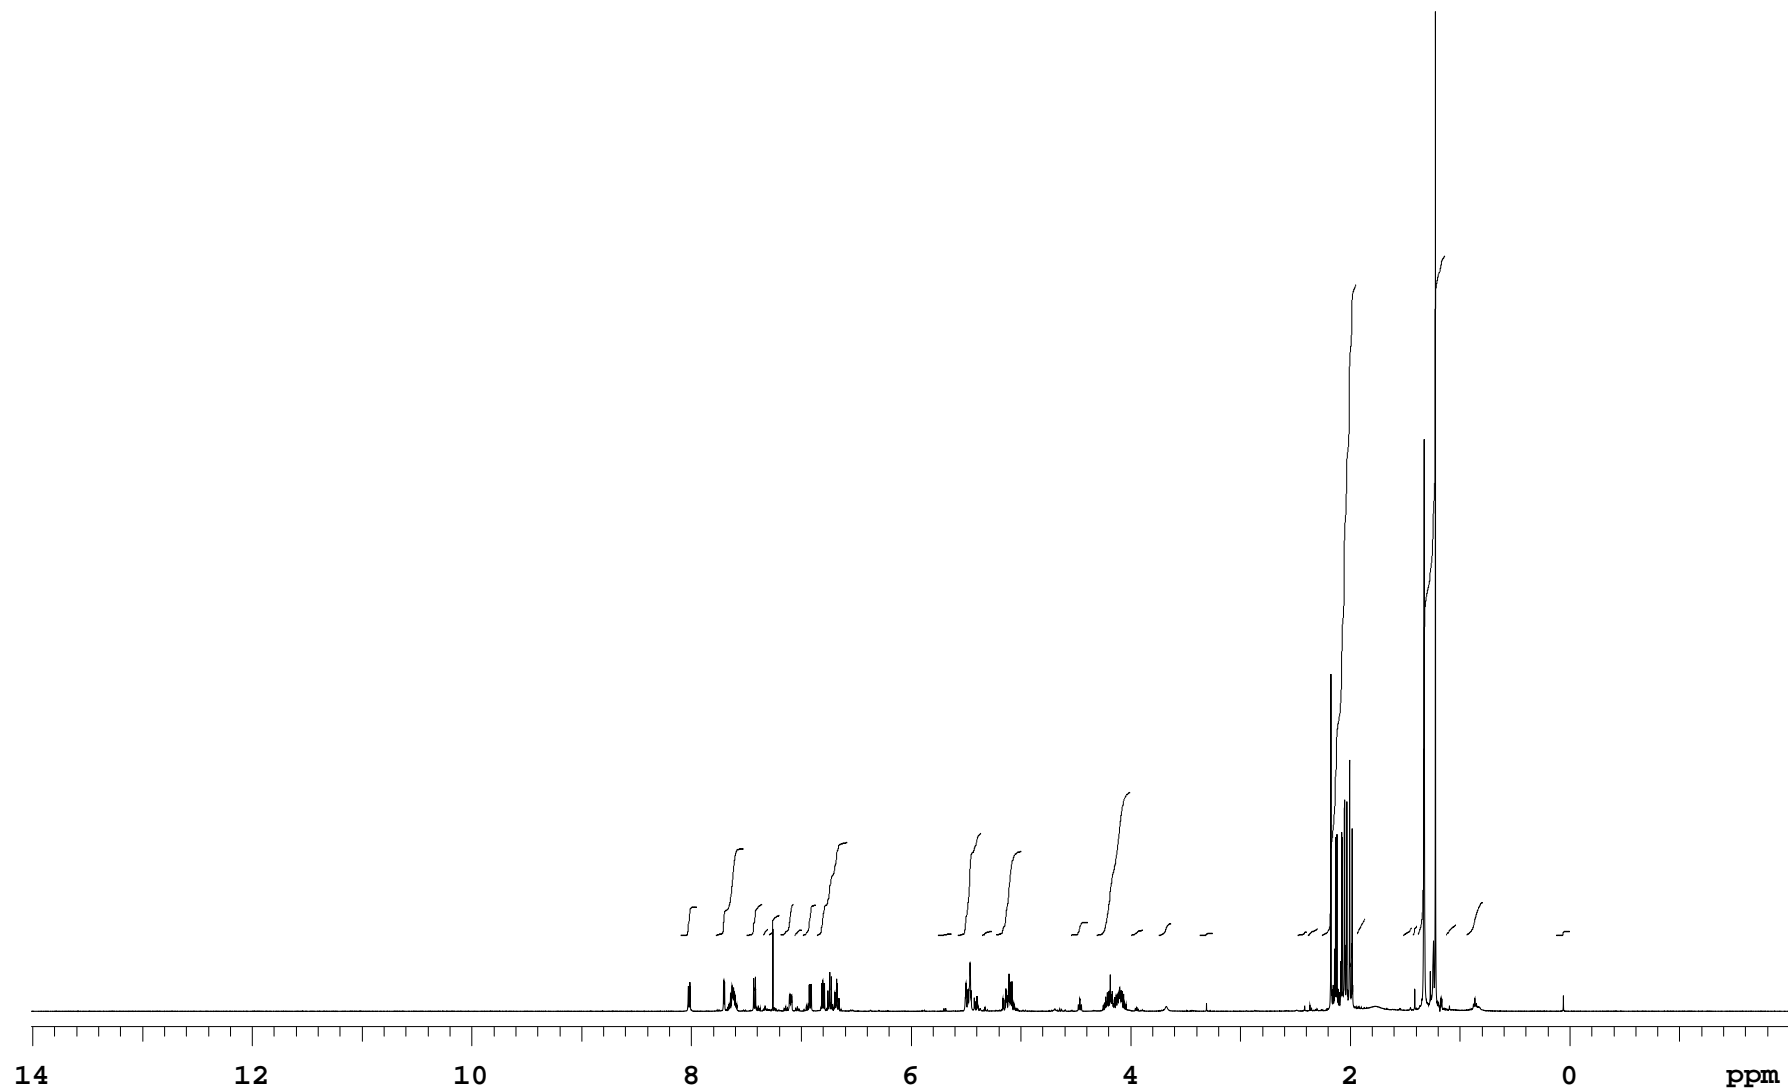

mlo162_column

Sample Name	mlo162_column	Pulse sequence	PROTON	Temperature	25	Study owner	mlo22
Date collected	2017-08-18	Solvent	cdcl3	Spectrometer	chpc-nmr500a-vnmrs500	Operator	mlo22

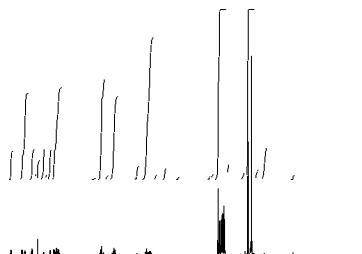

SAMPLE

date Aug 18 2017
 solvent cdcl3
 file /home/bath/vnmrsys
 /data/mlo22/mlo162_colum
 n_20170818_01/PROTON_01.
 fid

ACQUISITION

sw 8012.8
 at 2.045
 np 32768
 fb 4000
 bs 32
 d1 1.000
 nt 8
 ct 8

TRANSMITTER

tn H1
 sfrq 500.060
 tof 500.0
 tpwr 61
 pw 3.800

DECOUPLER

dn
 dof 0
 dm nnn
 decwave W40_HCN5mm
 dpwr 38
 dmf 32258

PRESATURATION

satmode n
 wet n

SPECIAL

temp 25.0
 gain 30
 spin 20
 hst 0.008
 pw90 7.600
 alfa 10.000

FLAGS

il n
 in n
 dp y
 hs nn

PROCESSING

fn 65536

DISPLAY

sp -1005.8
 wp 8012.6
 rfl 1006.1
 rfp 0
 rp 131.6
 lp 0

PLOT

wc 234
 sc 8
 vs 45
 th 44
 ai cdc ph

Plotname: PROTON_01_plot01

Data file /home/bath/vnmrsys/data/mlo22/mlo162_column_20170818_01/PROTON_01.fid

Plot date 2017-08-18