


krt38

Sample Name **krt38**  
Date collected **2018-07-09**

Pulse sequence **PROTON**  
Solvent **dms**

Temperature **25**  
Spectrometer **chpc-nmr500a-vnmrs500**

Study owner **mlo22**  
Operator **mlo22**

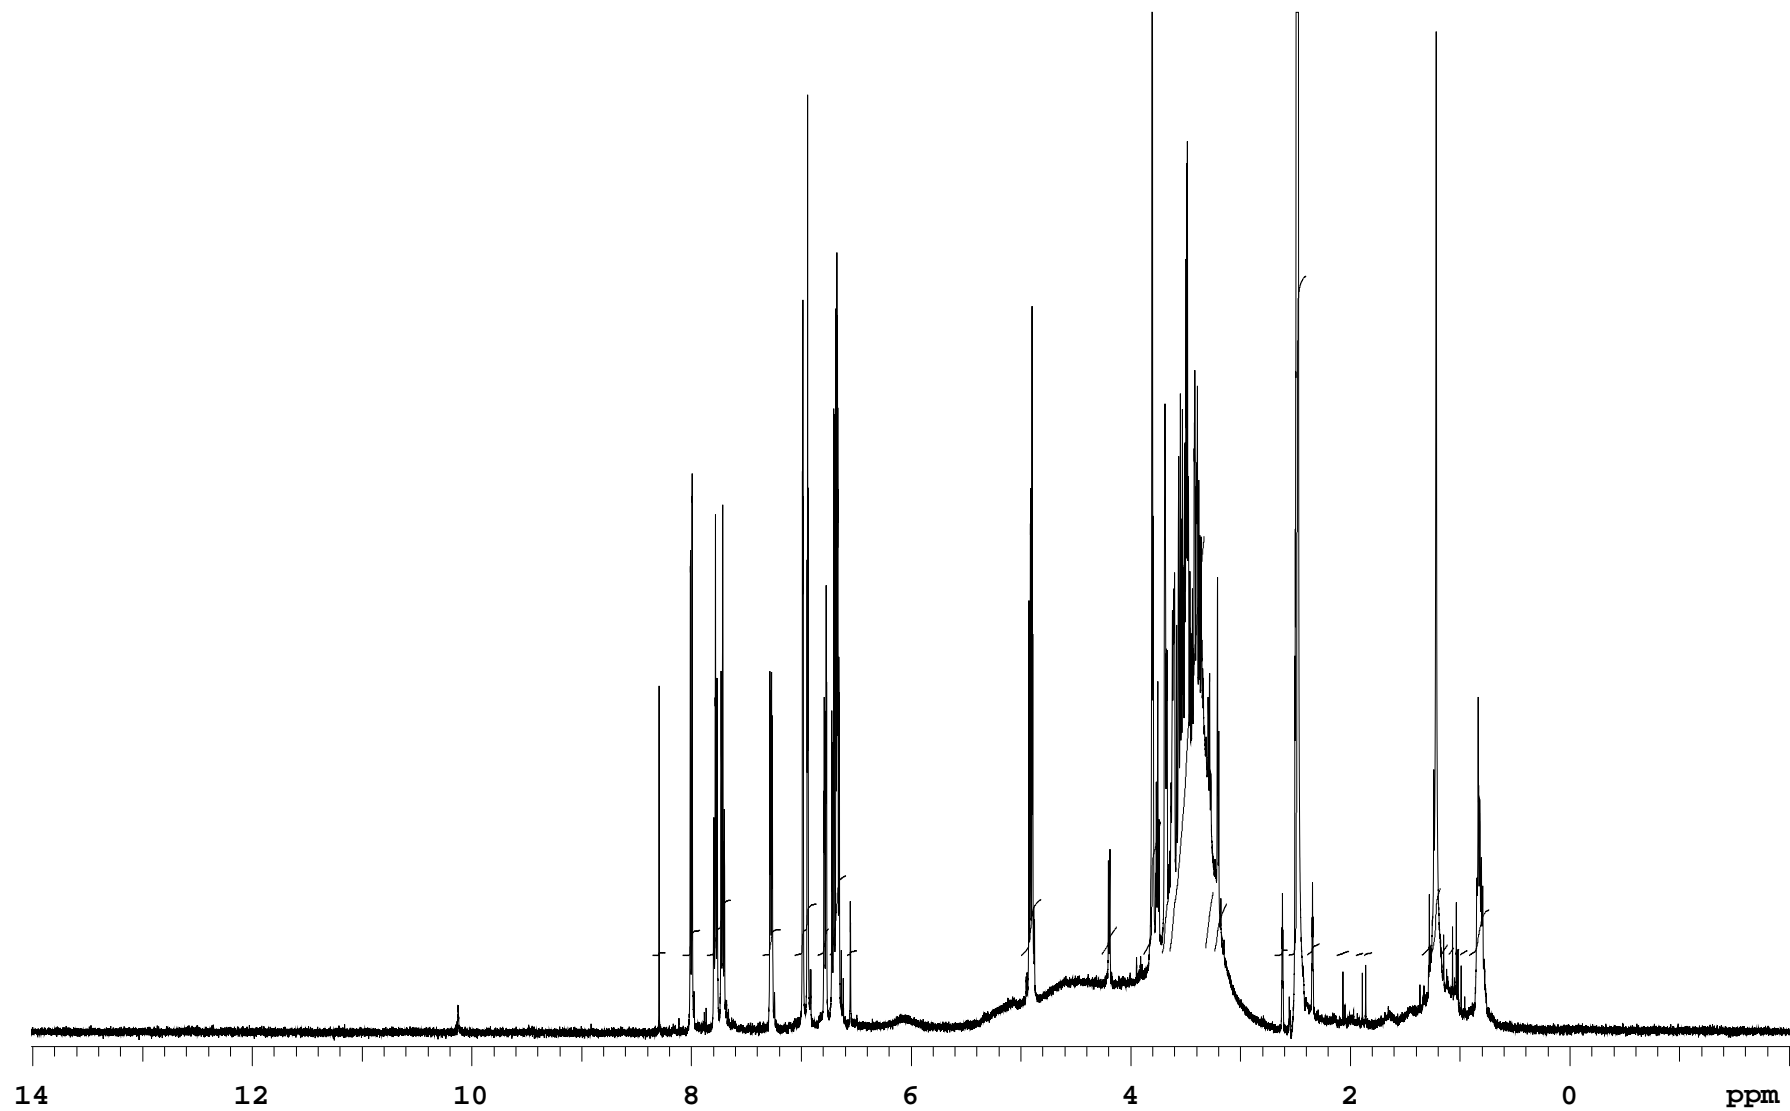


krt38

Sample Name **krt38**  
Date collected **2018-07-09**

Pulse sequence **PROTON**  
Solvent **dmsO**

Temperature **25**  
Spectrometer **chpc-nmr500a-vnmrs500**

Study owner **mlo22**  
Operator **mlo22**

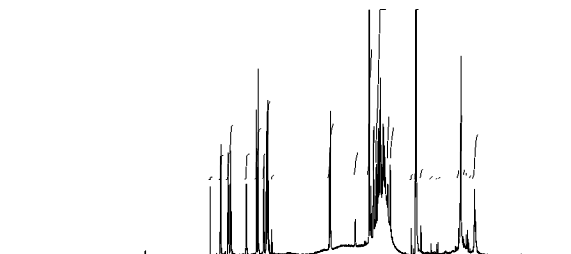

## INTEGRAL VALUES

Integral	start(ppm)	end	value
1	8.36176	8.23021	0.125
2	8.08204	7.9143	1.274
3	7.86638	7.63458	2.847
4	7.35731	7.18175	1.325
5	7.06145	6.85704	2.636
6	6.85704	6.74701	1.358
7	6.74652	6.58905	4.068
8	6.58905	6.48783	0.254
9	4.99631	4.81293	2.903
10	4.26914	4.1239	1.479
11	3.88624	3.72046	6.892
12	3.72046	3.65053	2.988
13	3.65053	3.32386	21.618
14	3.32337	3.24171	3.347
15	3.24171	3.1175	2.700
16	2.68911	2.56735	0.268
17	2.56686	2.39717	34.820
18	2.39717	2.27442	0.597
19	2.12625	2.00791	0.223
20	1.94971	1.87734	0.127
21	1.87734	1.79763	0.138
22	1.35017	1.26753	0.596
23	1.26704	1.17217	3.502
24	1.17217	1.10958	0.569
25	1.10958	1.05285	0.404
26	1.05236	1.0059	0.333
27	1.00541	0.929127	0.254
28	0.918368	0.729606	2.353

<b>SAMPLE</b>	wet	n
date	Jul 9 2018	
solvent	dmsO	
file	/home/bath/vnmrsys /data/mlo22/krt38_201807 09_01/PROTON_01.fid	
<b>ACQUISITION</b>	temp	25.0
	gain	40
	spin	0
	hst	0.008
	pw90	7.800
	alfa	10.000
<b>FLAGS</b>	il	n
sw	8012.8	
at	2.045	
np	32768	
fb	4000	
bs	32	
d1	1.000	
nt	8	
ct	8	
<b>PROCESSING</b>	fn	65536
<b>TRANSMITTER</b>	tn	H1
	sfrq	500.062
	tof	500.1
	tpwr	60
	pw	3.900
<b>DECOUPLER</b>	sp	-1005.8
	wp	8012.6
	rfl	1006.0
	rfp	0
	rp	-67.6
	lp	0
<b>PLOT</b>	dn	0
	dof	0
	dm	nnn
	decwave	W40_OneNMR
	dpwr	38
	dmf	32258
<b>PRESATURATION</b>	wc	234
	sc	8
	vs	1577
	th	2
	ai cdc ph	
satmode	n	

Plotname: PROTON\_01\_plot01

Data file /home/bath/vnmrsys/data/mlo22/krt38\_20180709\_01/PROTON\_01.fid

Plot date 2018-07-09